

FIG. 7

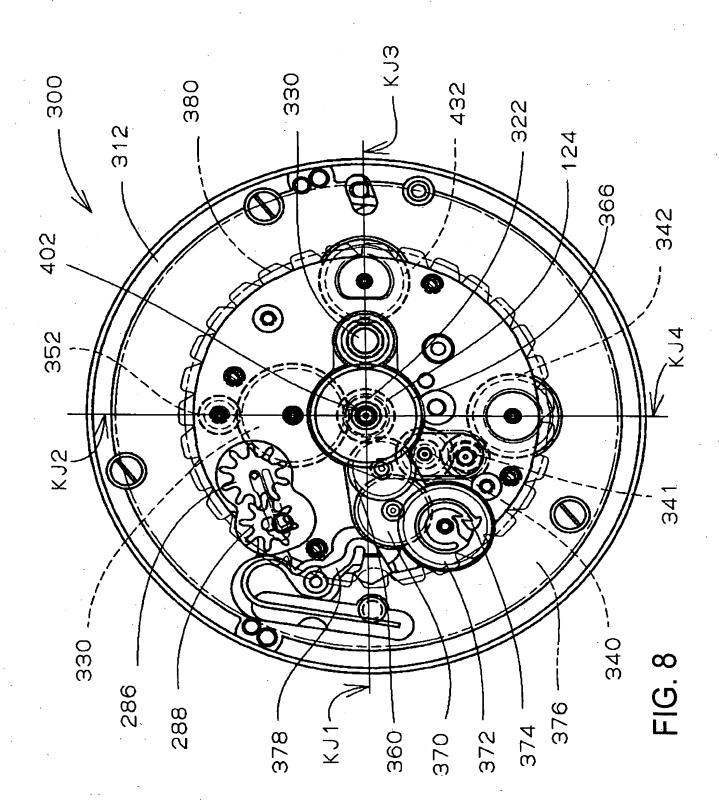
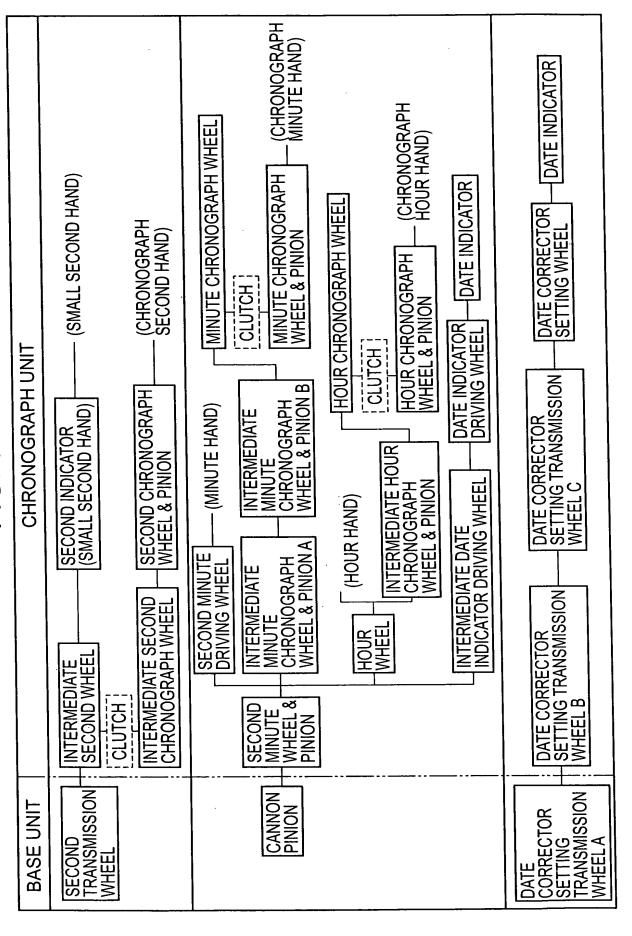
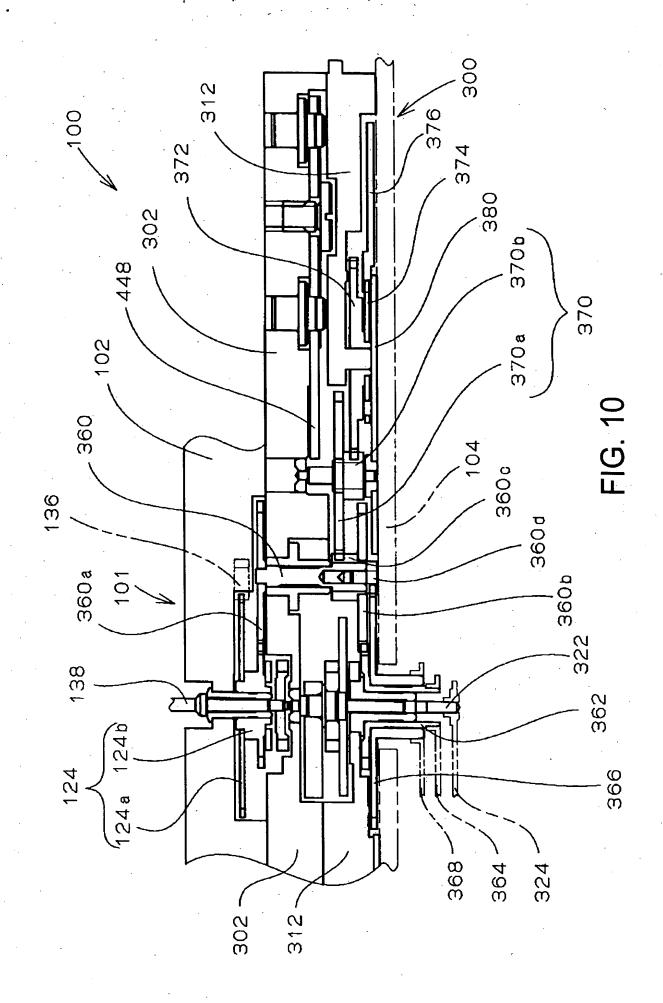
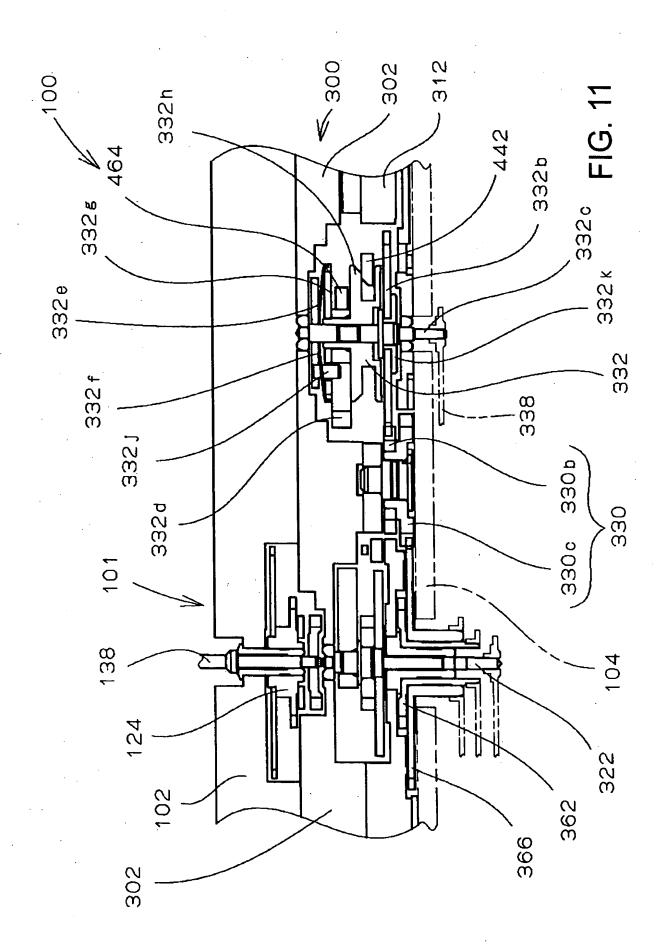
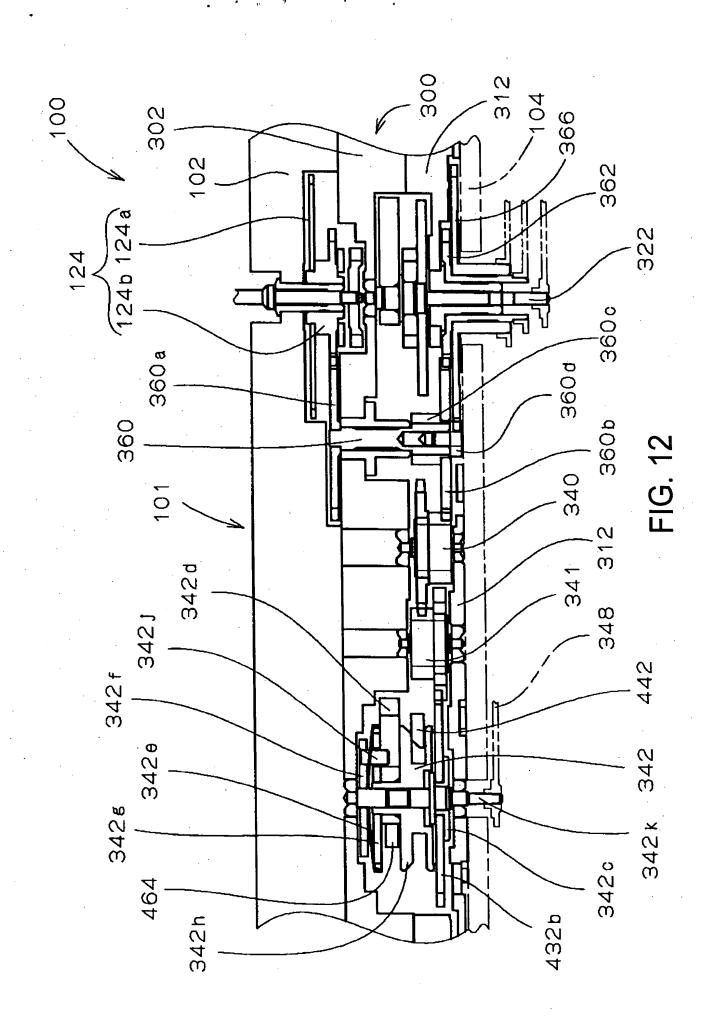



FIG. 9













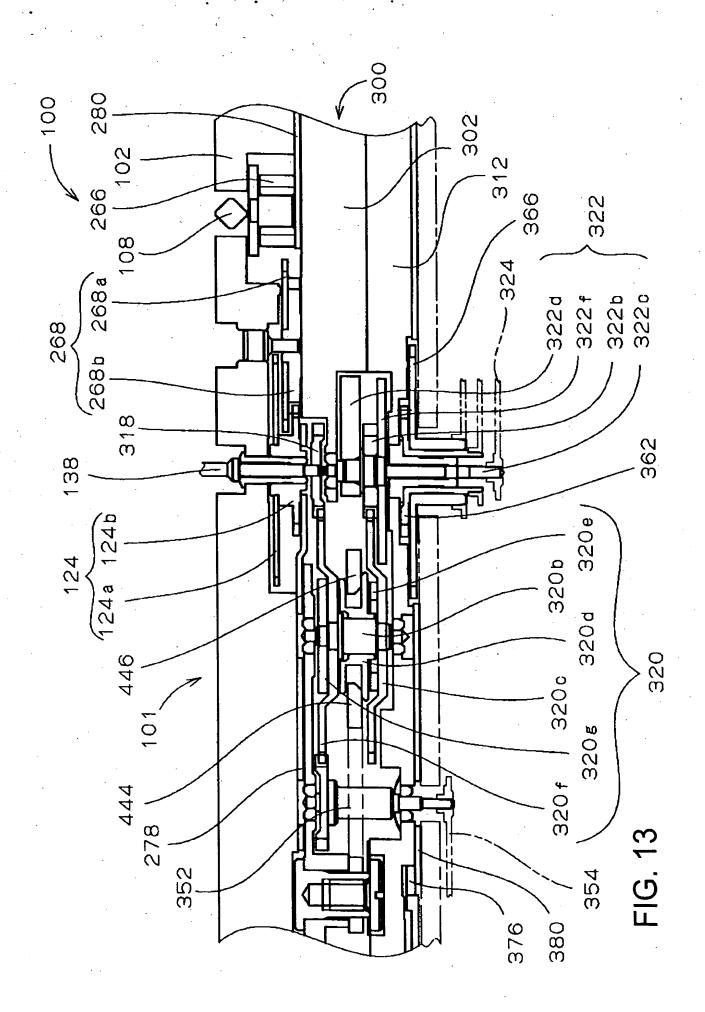


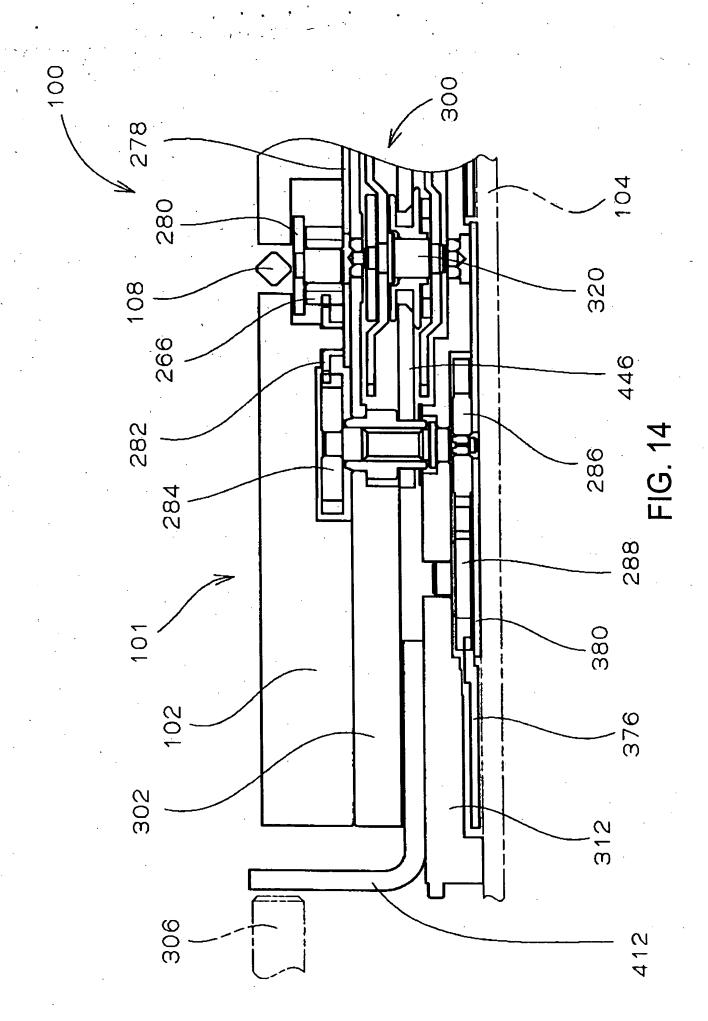


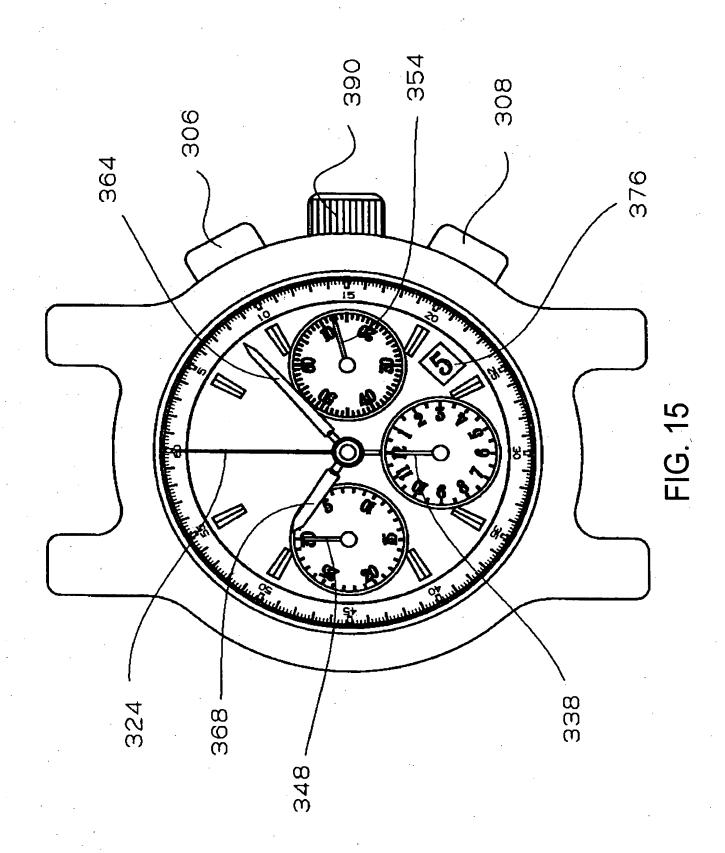


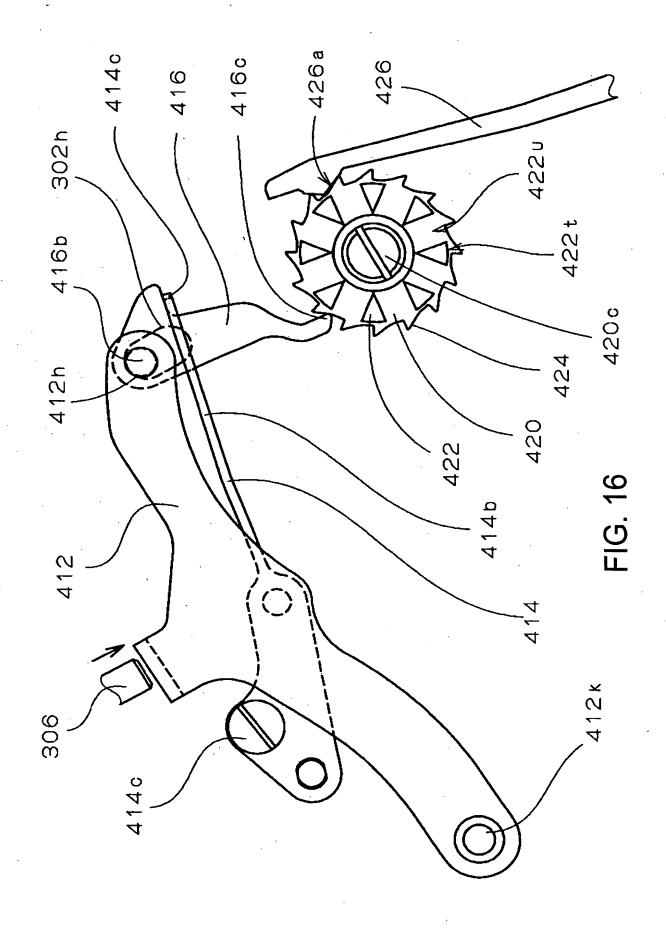


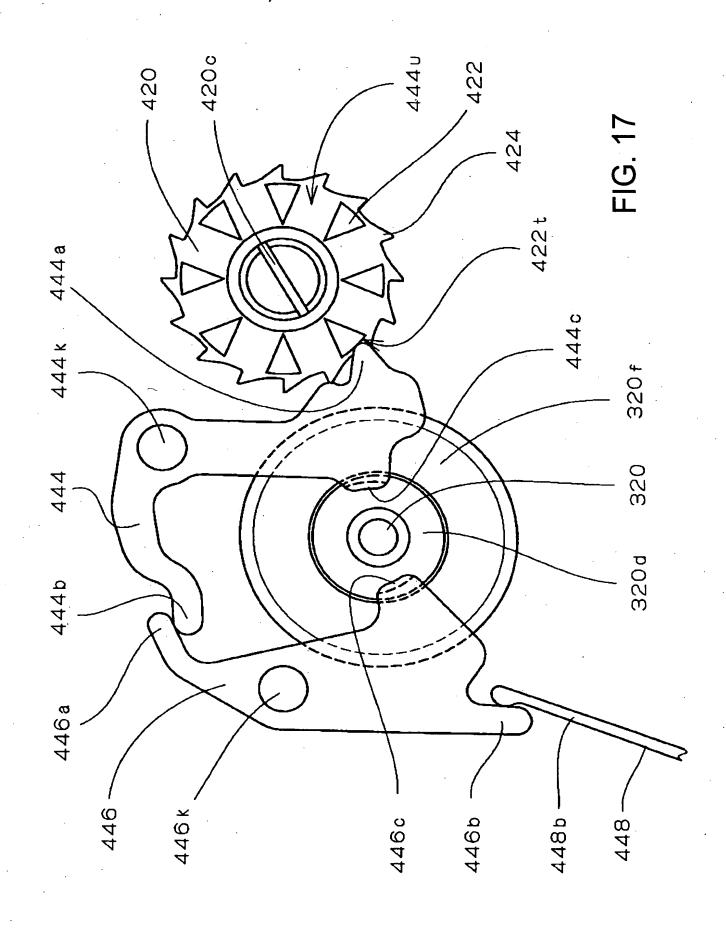


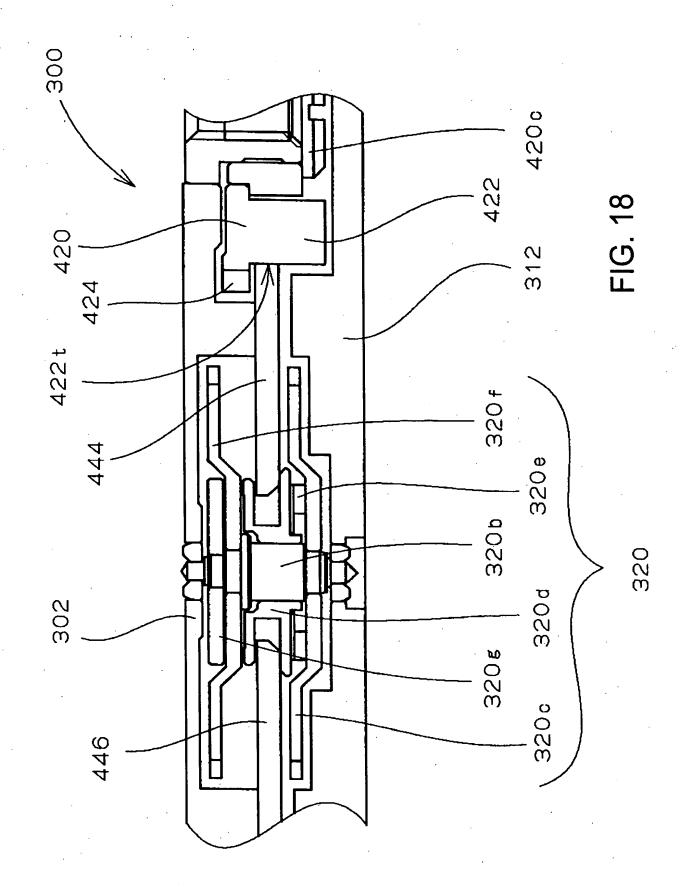

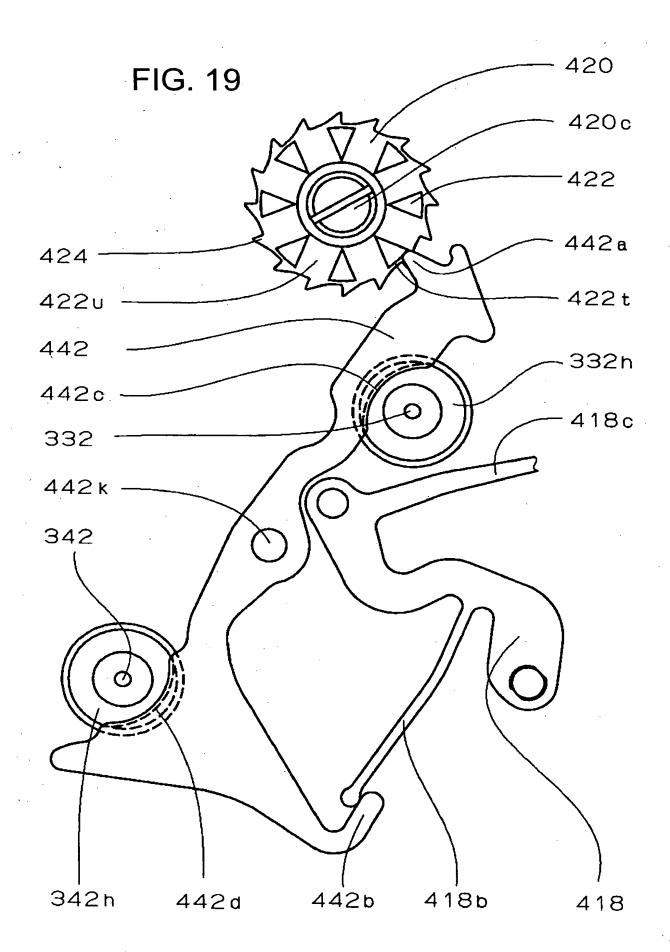

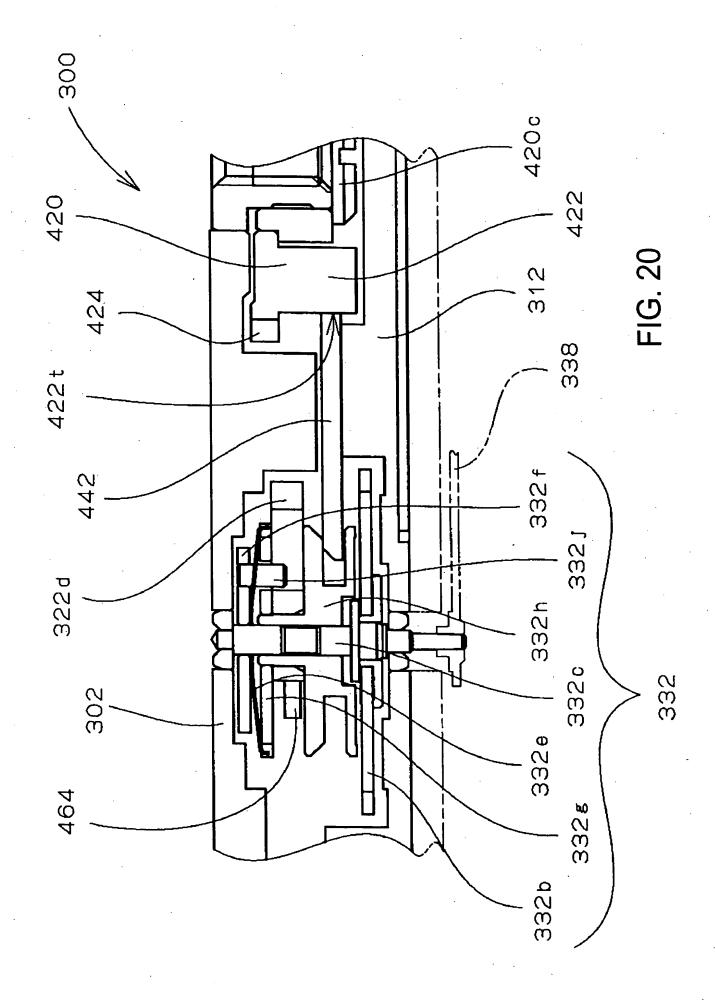

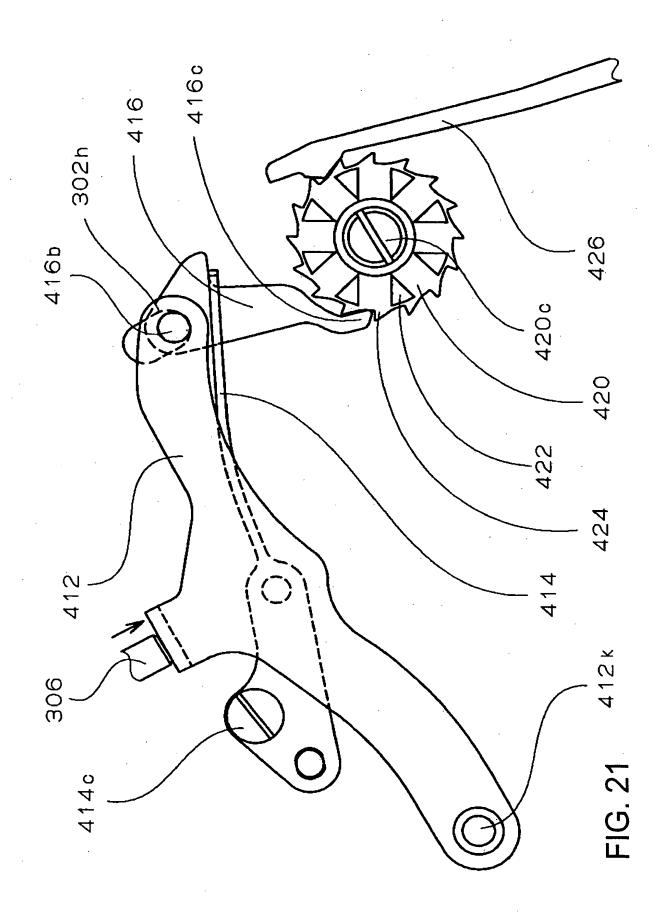

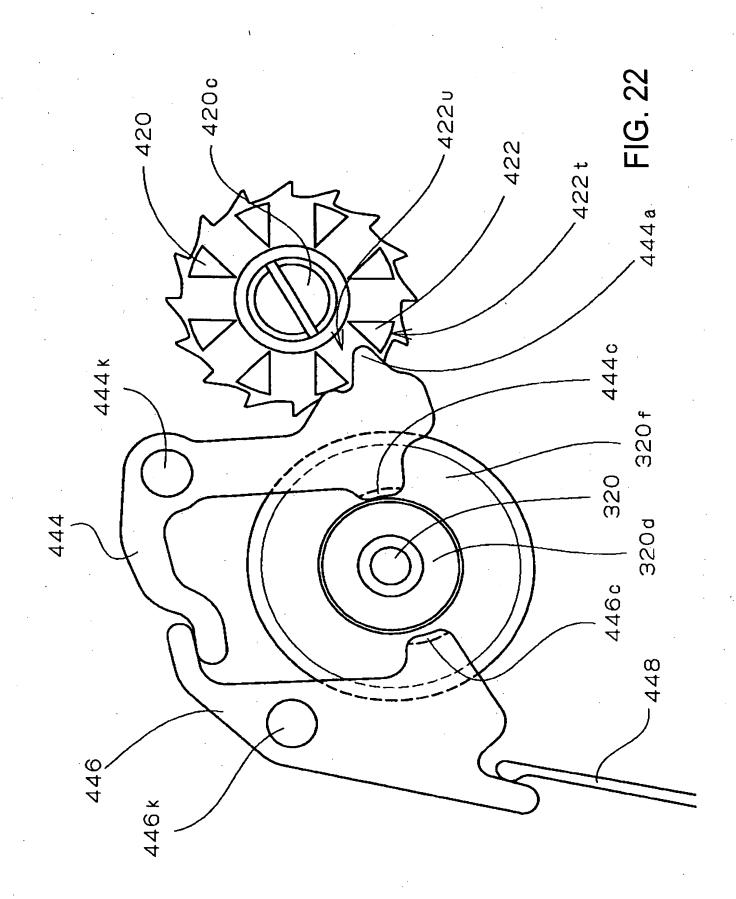

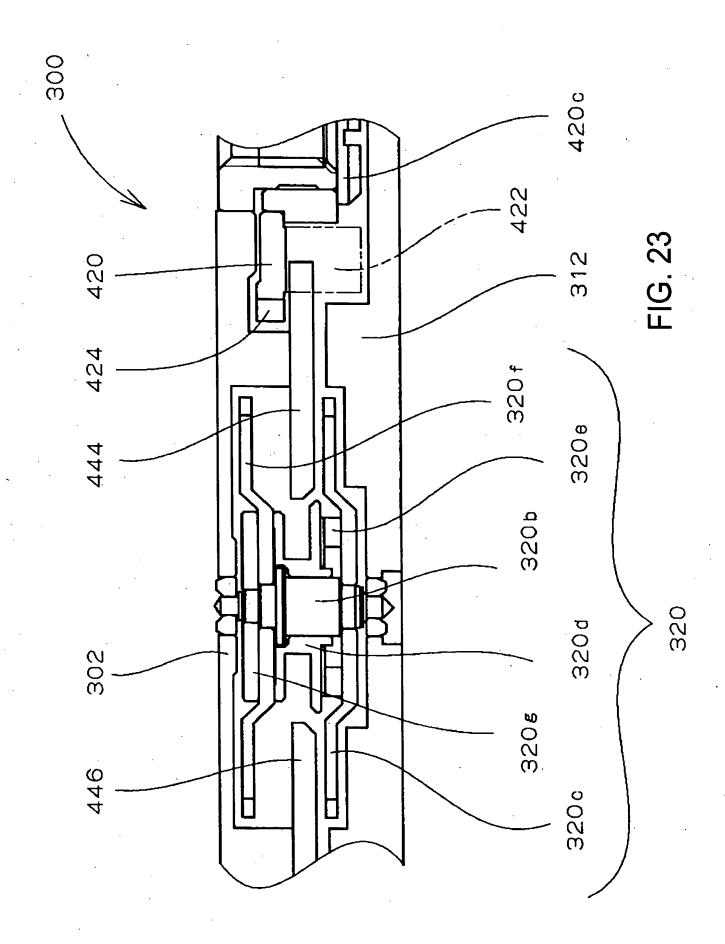
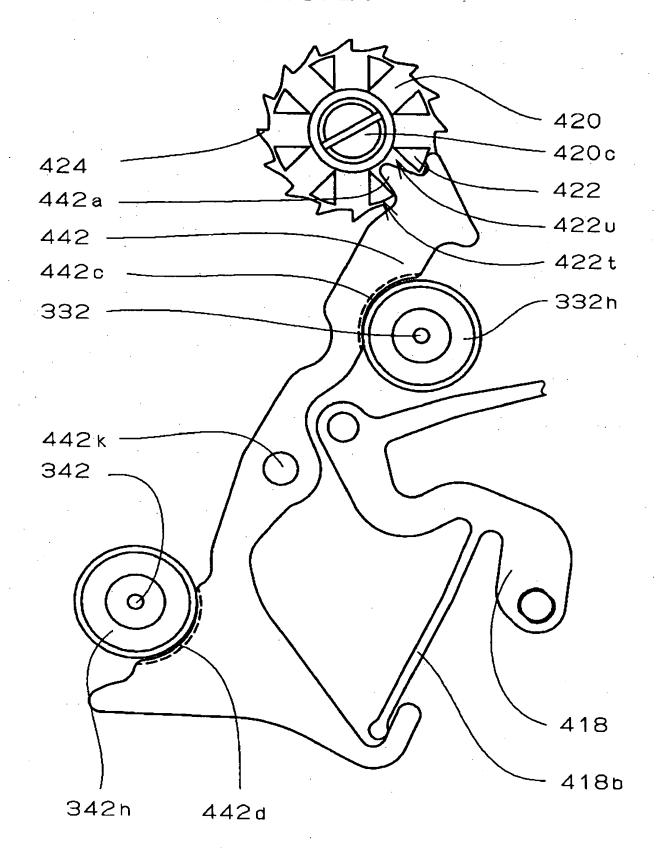
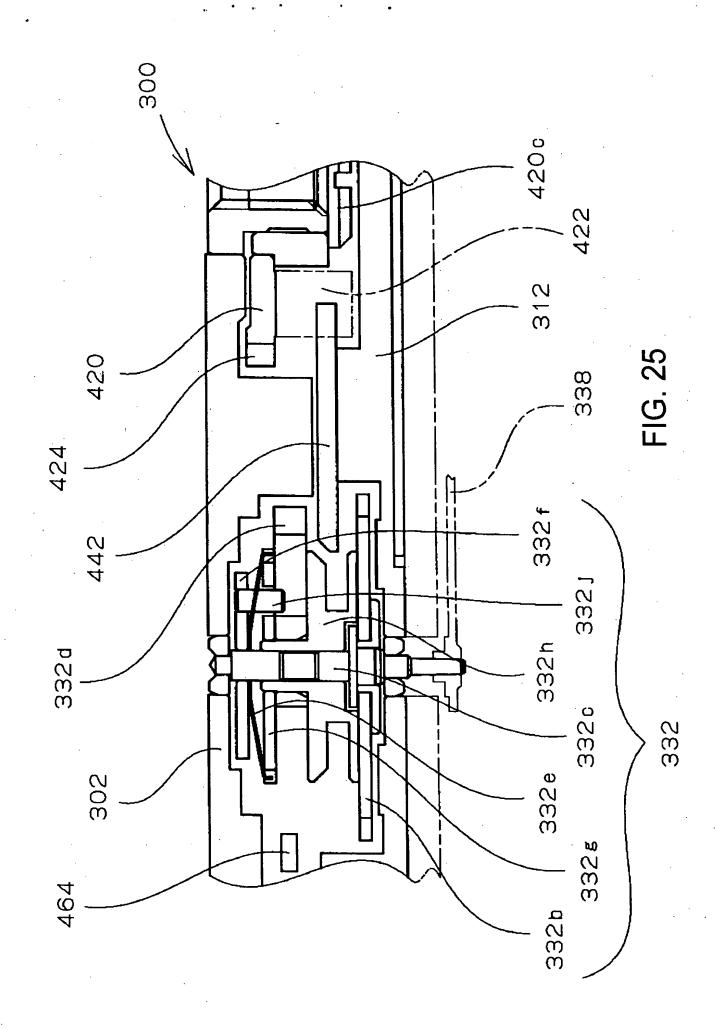


FIG. 24





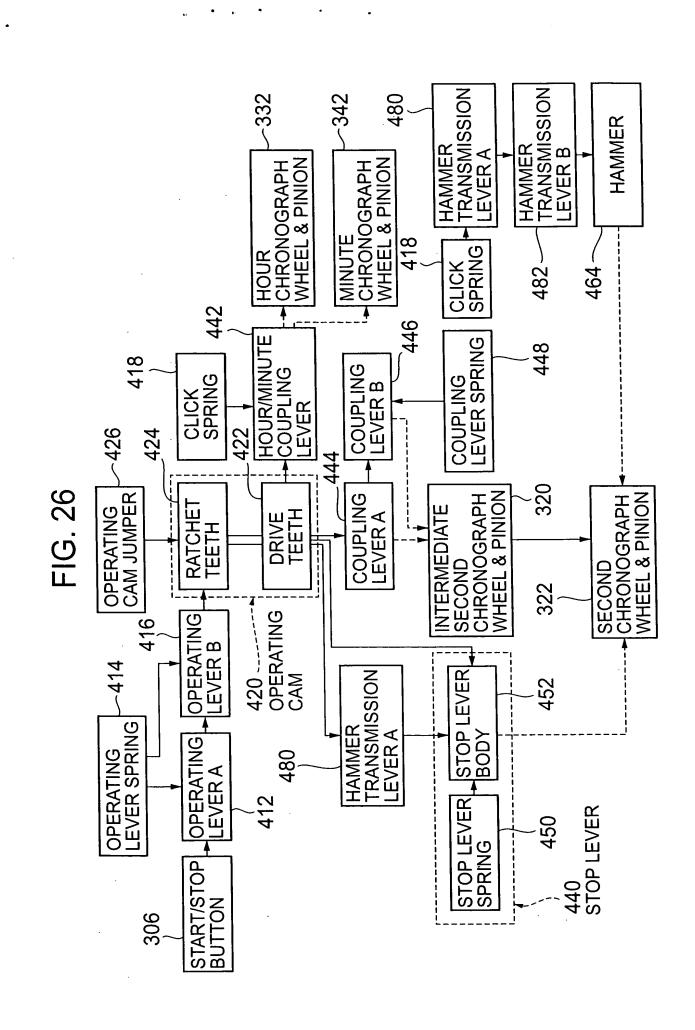
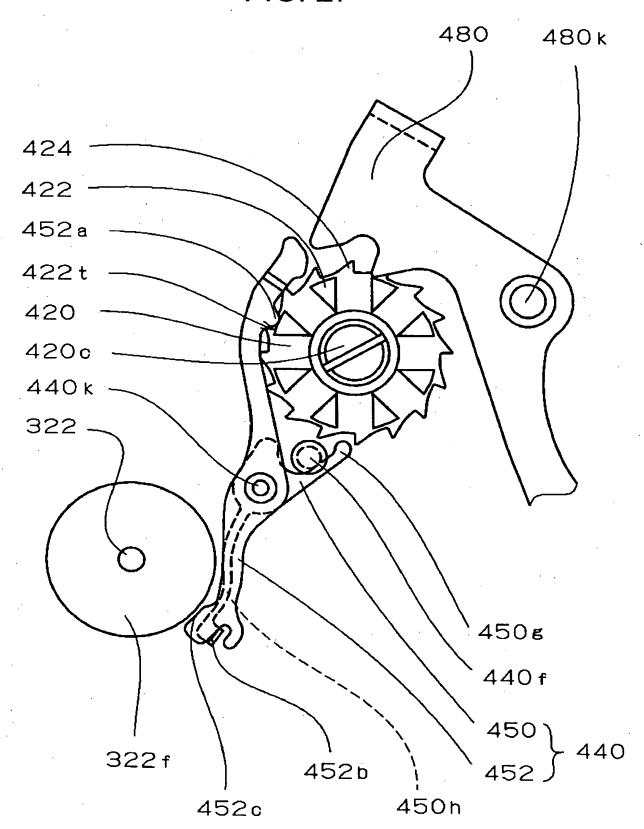


FIG. 27



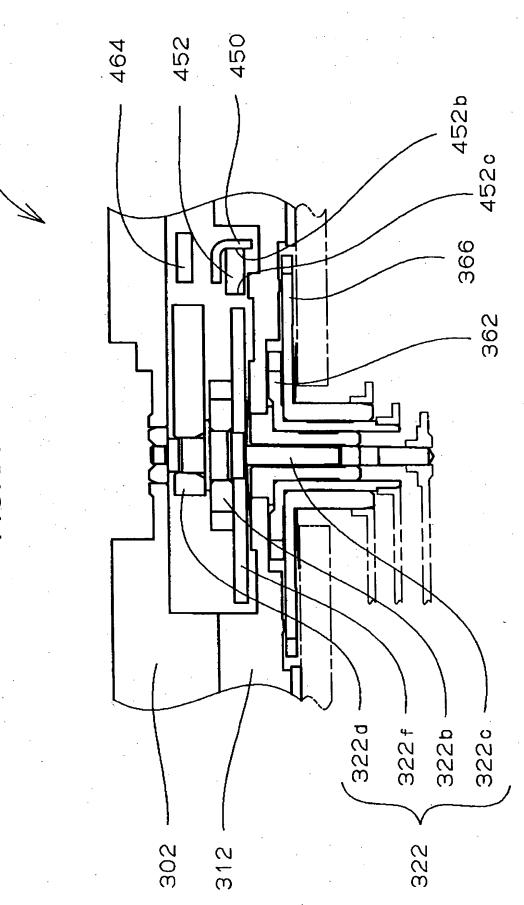
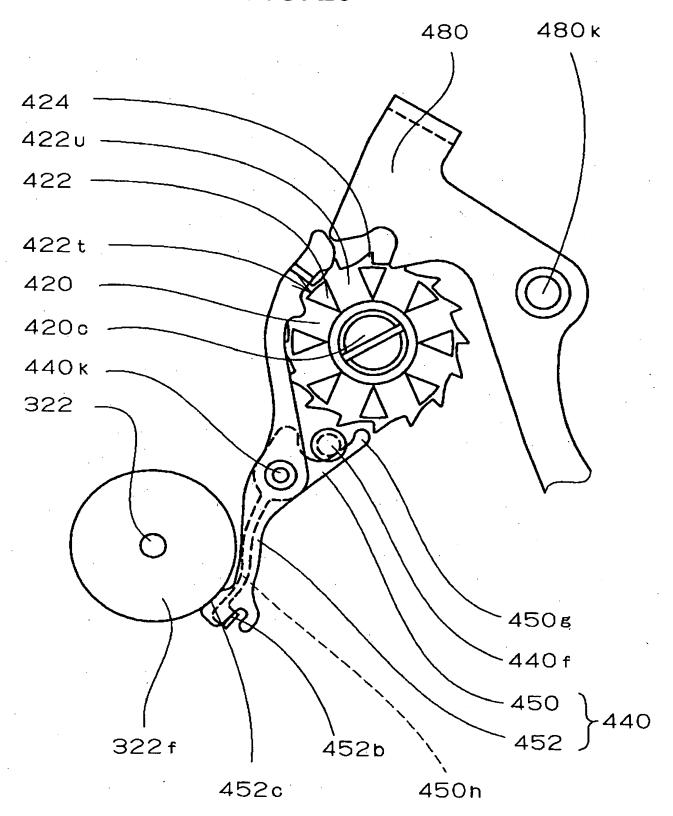


FIG. 28

300

FIG. 29



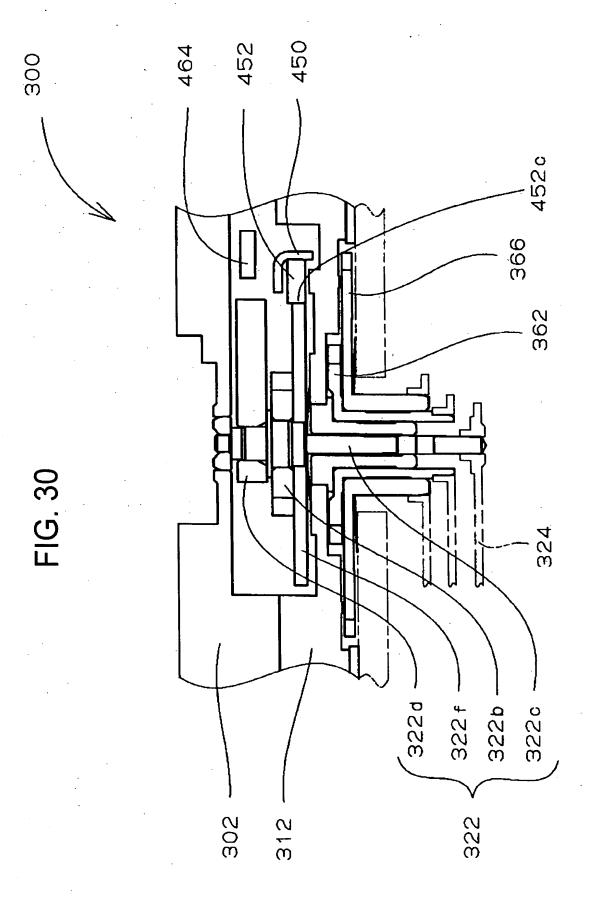
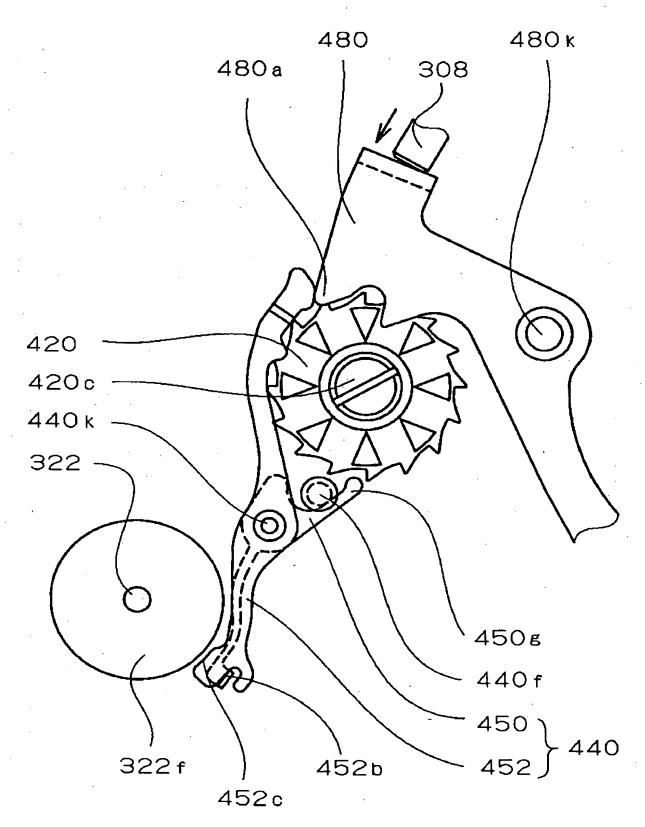


FIG. 31



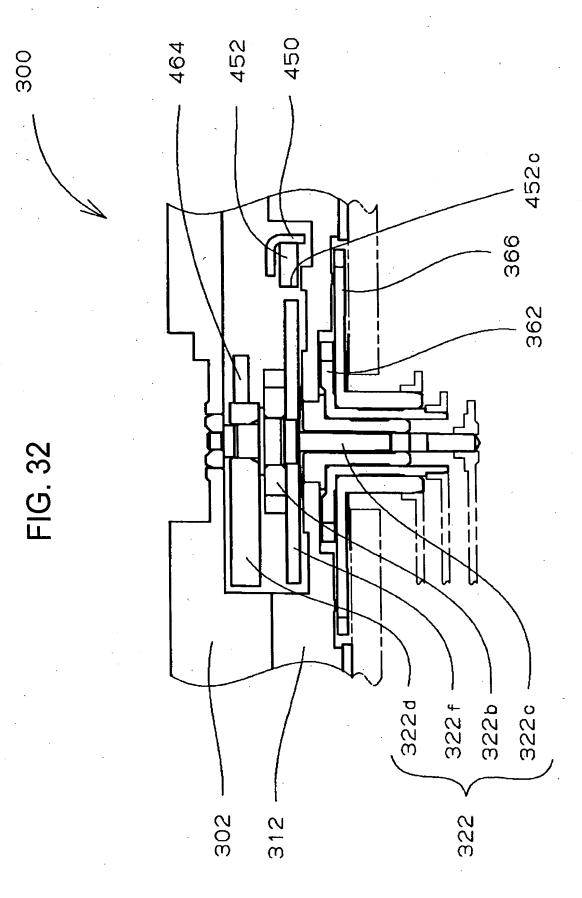


FIG. 33

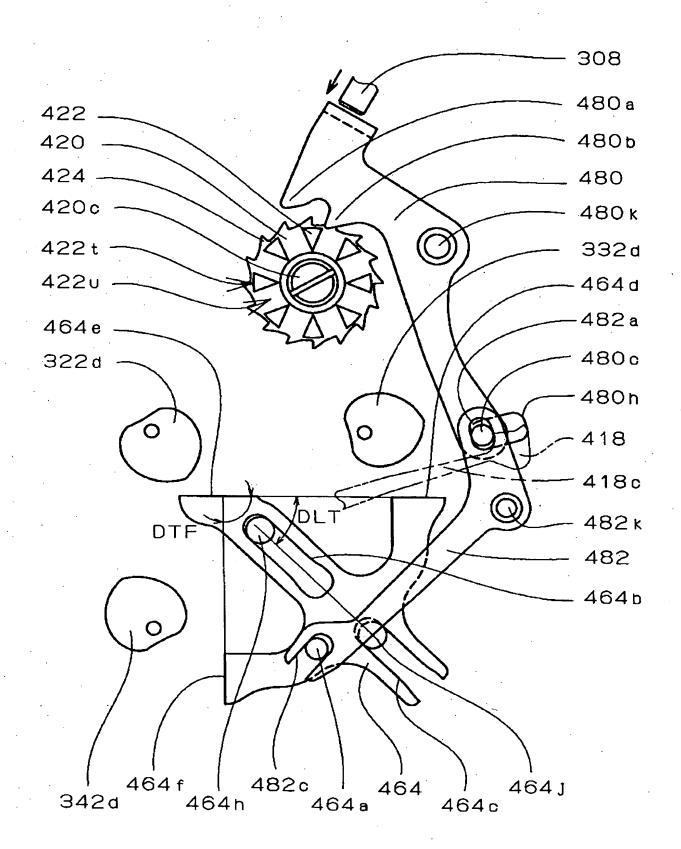


FIG. 34




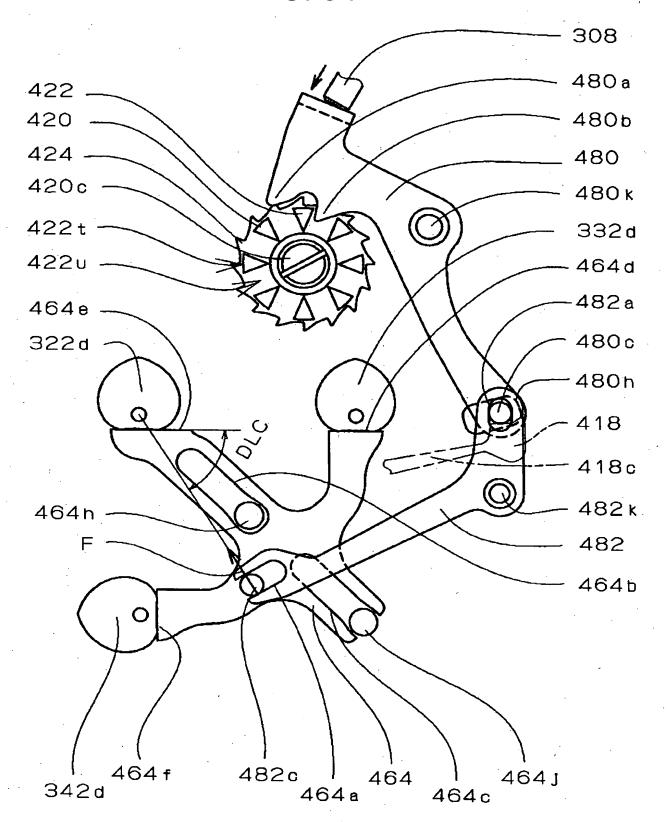


FIG. 35

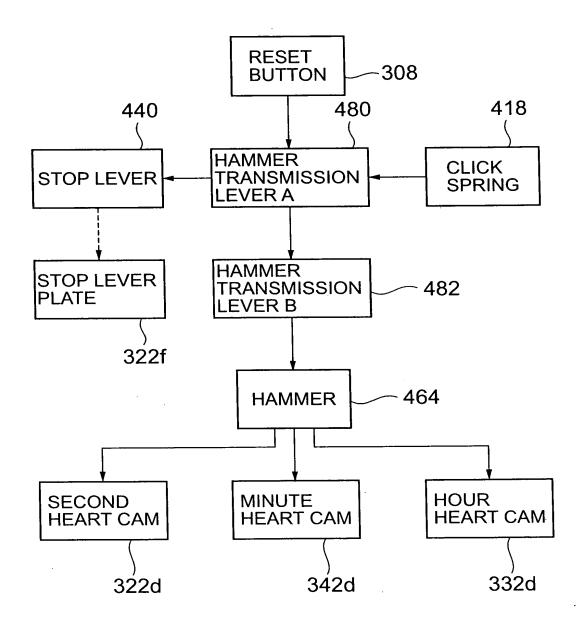

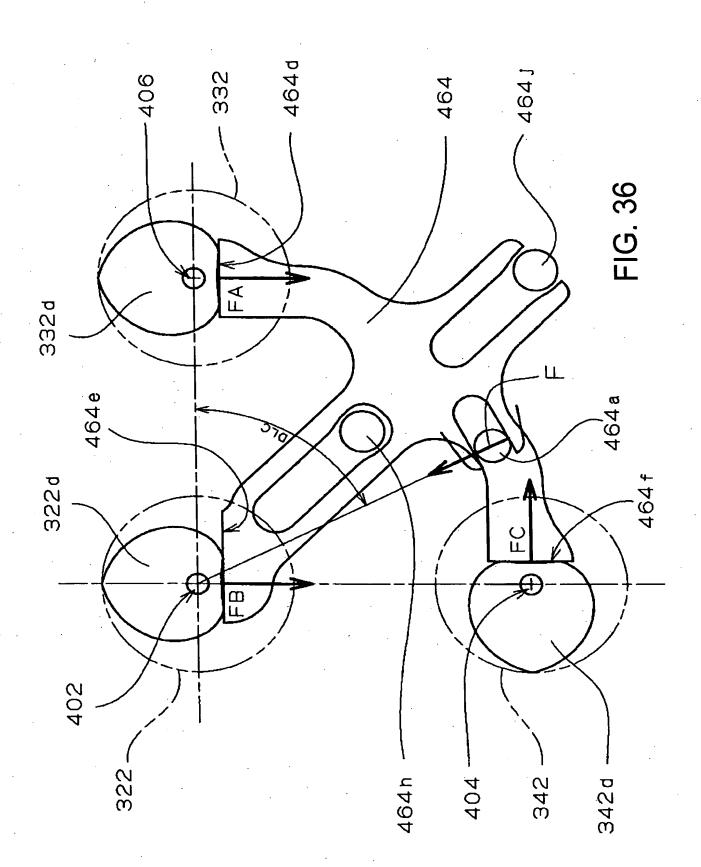

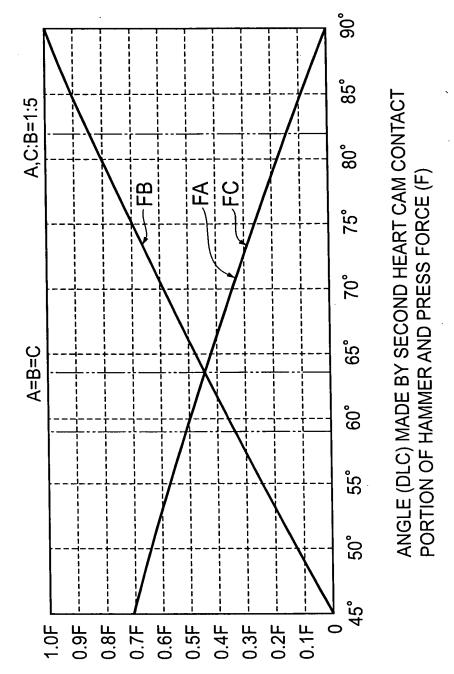

HEART CAM PRESSING FORCE (FA, FB, FC)